



نظام المشتريات والعطاءات

اسم العطاء : P1-2024  
وصف العطاء: مستهلكات أجهزة أكسدة الدم والرنة الصلاحية: الإصطناعية  
تاريخ إنشاء العطاء:  
الوثيقة المالية:  
طريقة الشراء:

Item No	Stock No	Stock Name	Quantity	Unit
1	20_09_232	Custom Pack Tubing Set to be Uesd with Oxygenator coated size Adult > or =50 kg	1900	Each
2	20_09_233	Custom Pack Tubing Set to be Uesd with Oxygenator coated size small - adult (25- 50) kg	120	Each
3	20_09_236	Oxygenator, Membrane Oxygenator Size Adult > or = 50 kg	1800	Each
4	20_09_238	Oxygenator, Membrane Oxygenator Size Small Adult ( 25 - 50) kg	190	Each

## شروط العطاء

## شروط خاصة

1-Goods must be dispatched/ delivered under the same storage conditions that comply with their nature; storage conditions must be mentioned clearly on all packages and relative documents.

2-Storage conditions as well as description of goods, lot no., expiry date and manufacturing date must be clearly indicated on all packages (inner and outer) and relative documents. If the manufacturing date is not applicable it must be provided on a separate document.

3-The delivered goods must be stamped, labeled or printed "sold to DRMS" Tender No. P1-2024, with irremovable ink.

4-All goods are to be freshly prepared on dispatch/ delivery & should have at least 2/3 of its shelf life upon receipt. Any item carrying less than 2/3 of its shelf upon receipt should be accompanied with a confirmation that you accept to replace any remaining unused quantities at your expenses after the expiry date. Said confirmation is subject to the approval of the director of the Royal Medical Services and will incur a fine, which will be decided later by DRMS according to the loss that this discrepancy with terms of the tender has caused.

5-All packages, parcels and related documents to be stamped or labeled with the following:

DRMS/TENDER (P1-2024)  
GHQ, JORDAN ARMED FORCES  
AMMAN – JORDAN

6-Goods must be previously evaluated and approved by DRMS or purchased by "Central procurement Branch" or by "Directorate of Defense procurement" tenders; RMS approval certificates (for previously approved items) should be submitted along with offers (this should be the responsibility of the bidders).

7-The following items should be delivered on (Free of charge) basis:

- For oxygenators: (6) holders size adult
- For custom packs: (6) holders size adult
- Temperature probes: (3) probes size adult.

---

8-The quality of the items should be according to the accepted international standards, i.e. (FDA, CE, or equivalent standard), accompanied with quality certificates.

9-Custom clearance of goods shall be the responsibility of the Jordan Armed Forces (JAF); however, suppliers shall bear all costs incurred by handling charges and any demurrage or extra expenses incurred by the port's corporation or QAIA (including expenses caused by delay in presenting the necessary shipment documents for either clearing or transporting the goods to the required location mentioned in the final order, delivery note issuing charges, unloading charges, local shipping charges etc.). The supplier is also responsible for providing of all relevant shipping documents, together with the delivery order(s).

10-Pricing must include services of sale, shipment, transportation, delivery from port to main medical stores.

11-The size, length, thickness and specifications of the tubes offered for custom packs should comply with the attached drawings.

12-Delivery/ shipment must be in two equal shipments (8-9) months apart.

✓13-For offers submitted in Jordanian Dinar, payment will be either by wire transfer or by bank check to be paid after receiving the documents from main medical stores. Any other way of payment will be rejected by the purchasing committee.


✓14-Bidders must submit their reservation/queries regarding tender specifications and/or special terms within the first half of the tender closing period starting from the tender announcement date, any reservation/queries submitted after the end of this period shall be rejected.

15-The estimated price for any (F.O.C) goods should be stated in the relative sheet.

16-The supplier or his local agent must furnish RMS with a guarantee stamped and legalized by the notary public equals to 115% of the total value of goods valid for (two years) after acceptance of goods.

17-After arrival to Jordan, DRMS is not responsible for any handling charges for goods (like charges for issuing delivery order for incoming shipment, unloading charges and local shipping agent's charges). In addition, GHQ/RMS are not responsible for any demurrage charges and any other charges incurred by the port's corporation or QAIA.

---

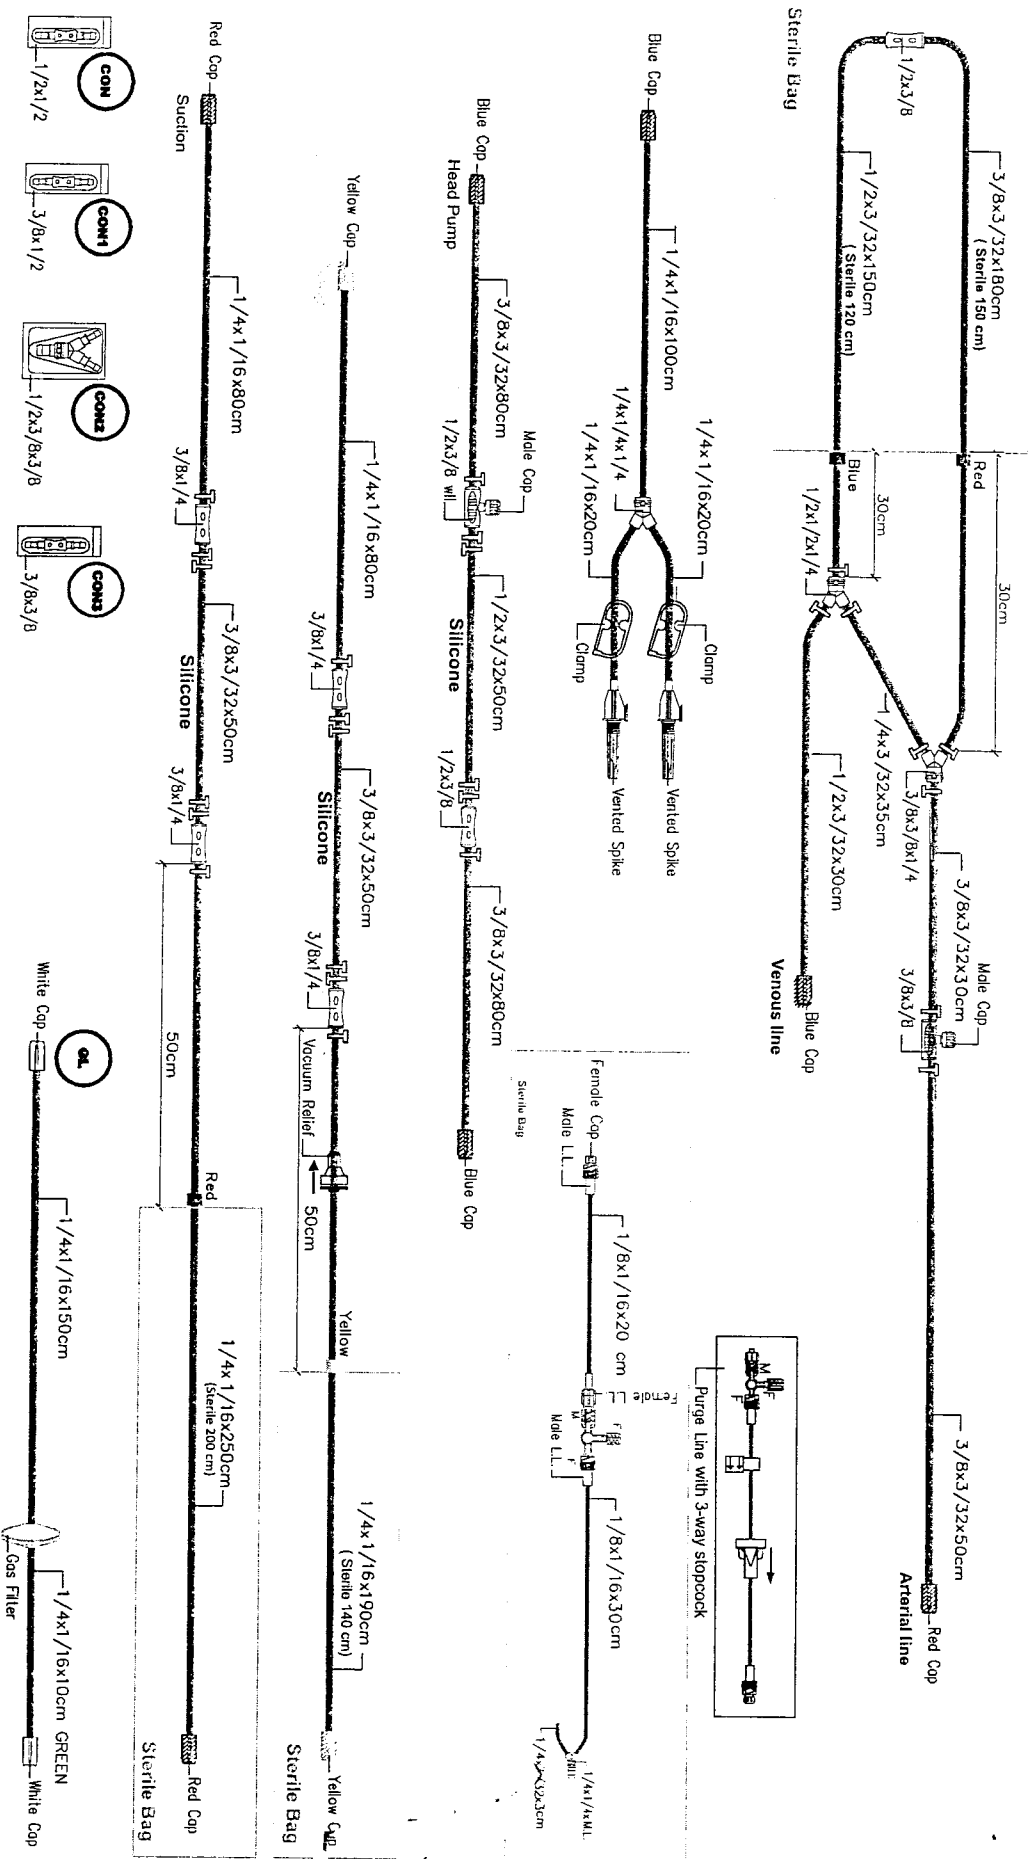






**PACKAGING:**

**Circuit Type:**  
**Adult Over 50 Kg** (Coating / Without filler)

**Country:** JORDAN  
**City:** AMMAN  
**Institution:** Royal Medical Services  
**Modified by:** Mohammad Ibrahim Barham, CCP.  
**Note:** The size and thickness of tubes should be labeled at the lines.  
**WLL :** With Luer lock.





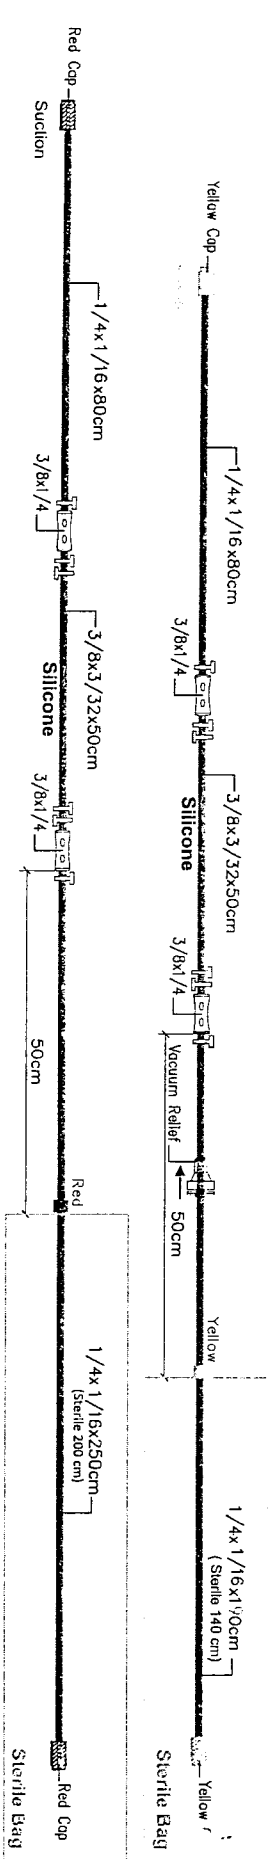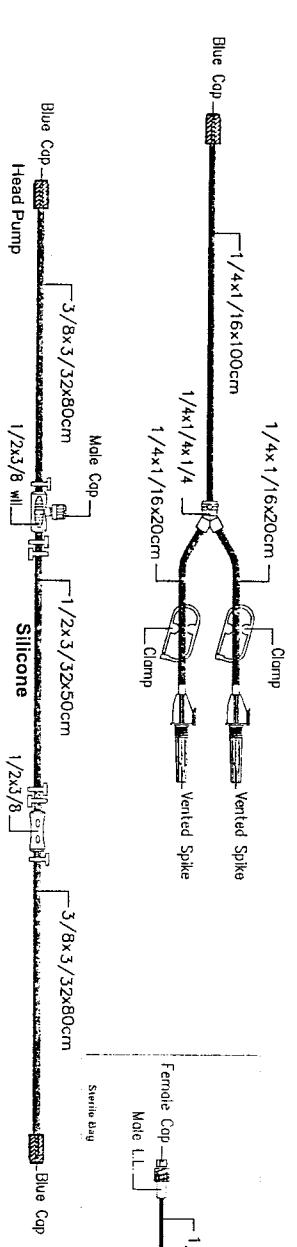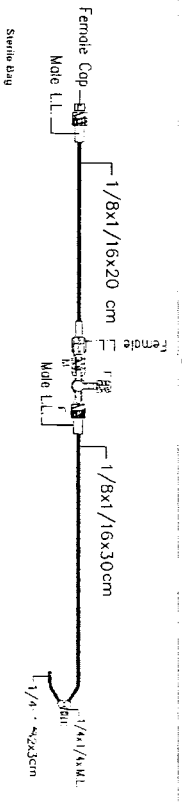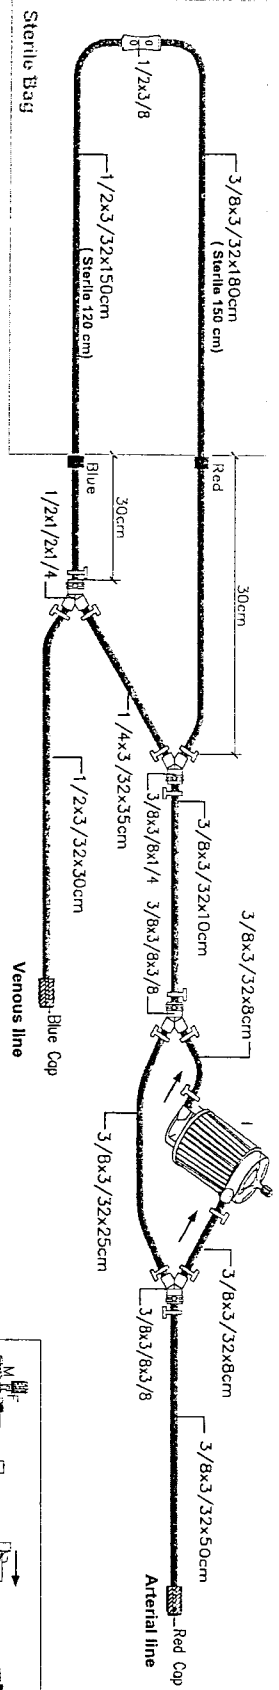

PACKAGING:

Circuit Type:  
Adult Over 50 Kg

Arterial Blood Filter Description:  
Maximum Flow ≥ 7000 ml/min  
Maximum Prime volume ≤ 220 ml  
Pore Diameter ≤ 40 μm

Country: JORDAN  
City: AMMAN  
Institution: Royal Medical Services

Modified by: Mohammad Ibrahim Barham, CCP.

Note:  
The size and thickness of tubes should be labeled at the lines.  
WLL : With Luer lock.

